


UR48  
PURGE  
300K



Current Data Parameters  
NAME urine-paper-160923  
EXPNO 34  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20160923  
Time 15.11 h  
INSTRUM spect  
PROBHD Z117768\_0063 (  
PULPROG zgpurge-gprefocus-4  
TD 65536  
SOLVENT urine  
NS 32  
DS 4  
SWH 12019.230 Hz  
FIDRES 0.366798 Hz  
AQ 2.7262976 sec  
RG 87.01  
DW 41.600 usec  
DE 42.44 usec  
TE 300.0 K  
D1 4.0000000 sec  
D16 0.0002000 sec  
D20 0.0002000 sec  
D21 0.0002000 sec  
TD0 1  
SFO1 600.1328246 MHz  
NUC1 1H  
P1 20.08 usec  
P2 40.16 usec  
PLW1 5.55840015 W  
PLW9 0.00008965 W  
GPNAM[1] SMSQ10.100  
GPZ1 -13.17 %  
GPNAM[2] SMSQ10.100  
GPZ2 52.68 %  
GPNAM[3] SMSQ10.100  
GPZ3 -17.13 %  
GPNAM[4] SMSQ10.100  
GPZ4 68.52 %  
P16 1000.00 usec

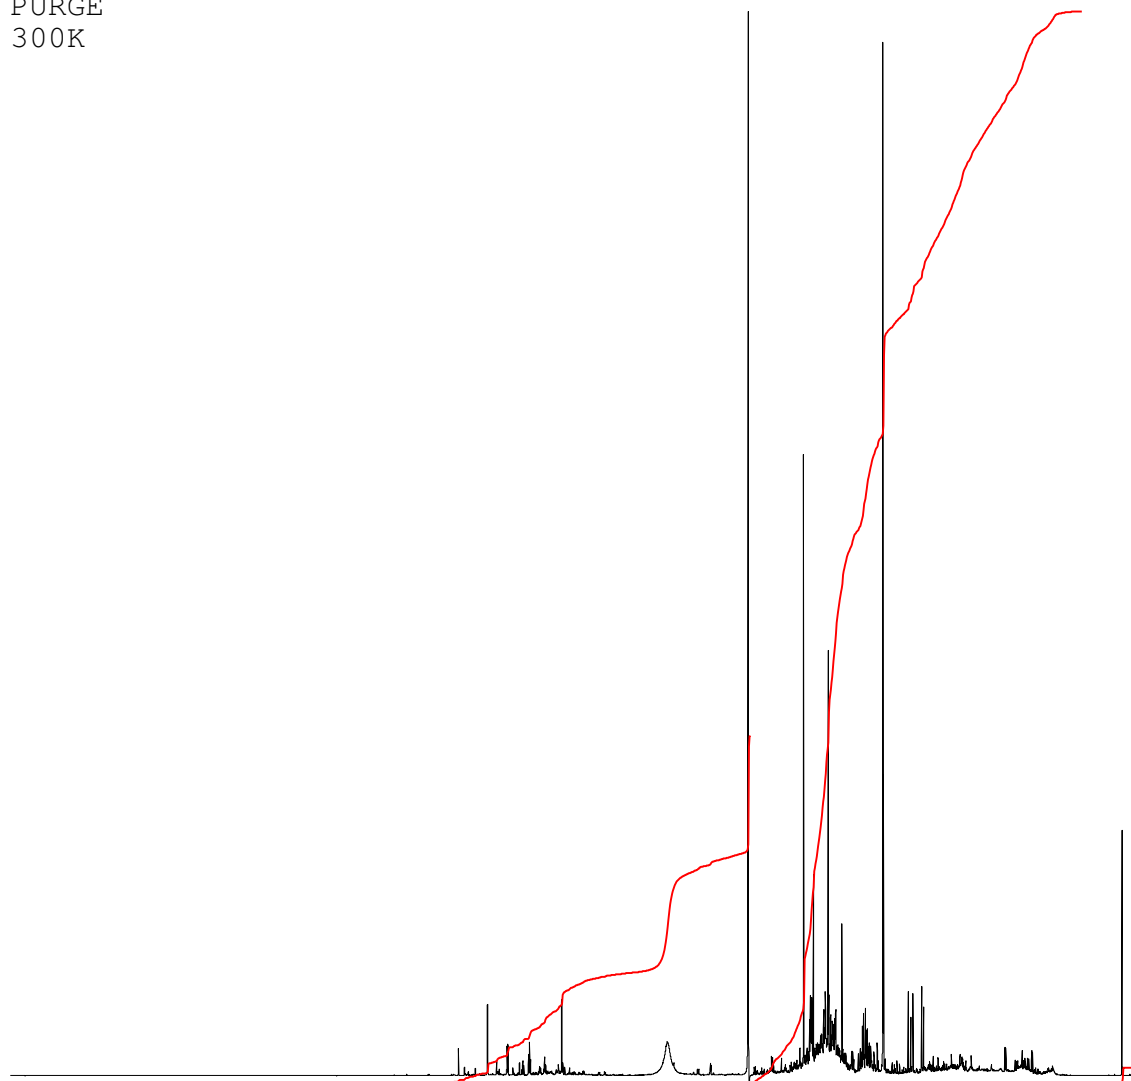

13 12 11 10 9 8 7 6 5 4 3 2 1 0 -1 -2 -3 ppm

24.14 74.80 1.06

F2 - Processing parameters  
SI 65536  
SF 600.1299594 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 0